

Molecular Innovations, Inc.

46430 Peary Court
Novi, MI 48377
TEL: (248) 896-0142
FAX: (248) 896-0148
<http://www.mol-innov.com>

Certificate of Analysis

Product: Human Ceruloplasmin Antigen ELISA kit – HCPKT

Lot: HCPKT-816

Date of Manufacture: 5 August 2016

Expiration Date: 30 August 2018

Components:

Instruction/Reagent Sheet	Number of copies: 1	Lot #: HCPKT-816
ELISA Plate	Number of plates: 1	Lot #: 816C
10X Wash Buffer	Number of vials: 1	Lot #: 816
1,000ng/ml Standard	Number of vials: 1	Lot #: 416L
Primary Antibody	Number of vials: 1	Lot #: 416L
Secondary Reagent	Number of vials: 1	Lot #: SAVI-HRP-816
Substrate	Number of vials: 1	Lot #: 15299-A

Test

Average Background OD
Average High OD
Development Time



Specification

≤ 0.15
 ≥ 1.0
 ≤ 10 minutes

Result

0.065
1.69
6 minutes

Quality Control Standard Curve:

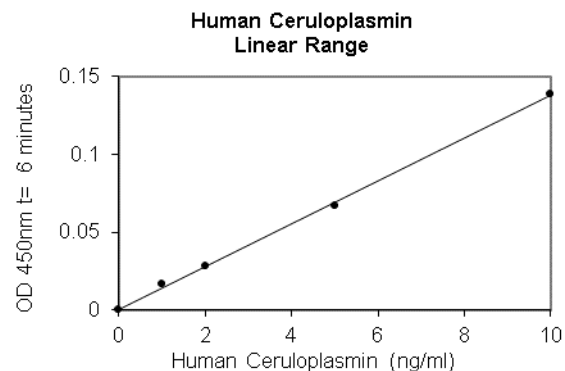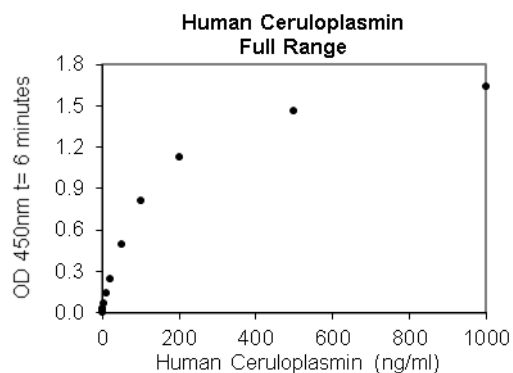

Duane E. Day

Duane E. Day