

## Molecular Innovations, Inc.

46430 Peary Court  
Novi, MI 48377  
TEL: (248) 896-0142  
FAX: (248) 896-0148  
<http://www.mol-innov.com>

# Certificate of Analysis

**Product:** Human Prekallikrein Total Antigen ELISA kit – HPKKT-TOT

**Lot:** HPKKT-TOT-1216

**Date of Manufacture:** 12 December 2016

**Expiration Date:** 31 December 2018

### Components:

Instruction/Reagent Sheet	Number of copies: 1	Lot #: HPKKT-TOT-1216
ELISA Plate	Number of plates: 1	Lot #: 1116C
10X Wash Buffer	Number of vials: 1	Lot #: 1216
10µg/ml Standard	Number of vials: 1	Lot #: 116L
Primary Antibody	Number of vials: 1	Lot #: 311L
Secondary Antibody	Number of vials: 1	Lot #: DAS-HRP-816
Substrate	Number of vials: 1	Lot #: 16185-B

### Test

Average Background OD  
Average High OD  
Development Time



### Specification

≤ 0.15  
≥ 1.0  
≤ 10 minutes

### Result

0.078  
2.95  
4.5 minutes

### Quality Control Standard Curve:

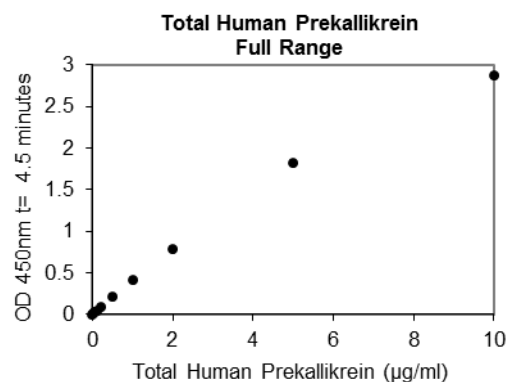

*Duane E. Day*

Duane E. Day