

Molecular Innovations, Inc.

46430 Peary Court
Novi, MI 48377
TEL: (248) 896-0142
FAX: (248) 896-0148
<http://www.mol-innov.com>

Certificate of Analysis

Product: Mouse PAI-1 total antigen assay ELISA kit – MPAIKT-TOT

Lot: MPAIKT-TOT-416

Date of Manufacture: 8 April 2016

Expiration Date: 28 April 2018

Components:

Instruction/Reagent Sheet	Number of copies: 1	Lot #: MPAIKT-TOT-416
ELISA Plate	Number of plates: 1	Lot #: 416C
10X Wash Buffer	Number of vials: 1	Lot #: 416
250ng/ml Standard	Number of vials: 1	Lot #: 415L
Primary Antibody	Number of vials: 1	Lot #: 415L
Secondary Antibody	Number of vials: 1	Lot #: GAR-HRP-316
Substrate	Number of vials: 1	Lot #: 15299-A

Test

Average Background OD
Average High OD
Development Time



Specification

≤ 0.15
 ≥ 1.5
 ≤ 10 minutes

Result

0.0545
3.65
2 minutes

Quality Control Standard Curve:

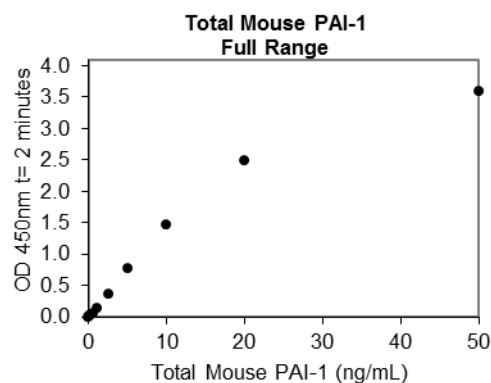

Duane E. Day

Duane E. Day